



Ultrasonic Scaler Instruction Manual

(For PT 7)

Please read this manual before operating

Guilin Refine Medical Instrument Co., LTD.

RF-PT7-M004 Version: 1.4 20230203

<https://www.kadashika.jp>

Contents



























1 Product introduction	2
2 Installation and adjustment	3
3 Scaling & periodontal treatment function and use	4
4 Troubles shotted	5
5 Cleaning, disinfecting and sterilizing	7
6 Transportation, Storage And Maintenance	7
7 Environmental protection	8
8 EMC - Declaration of conformity	8
Attachment. Reprocessing instructions of cleaning, disinfecting and sterilizing	12

Safety Precautions

 **WARNING: If you neglect these safety precautions, you may cause personal injury such as electric shock, fire or damage to the product.**

1. Use a separate, grounded power outlet. Never use wet hands to unplug the power cord.
2. Please put the power plug into the socket easy to pull out, to make sure it can be pulled out in emergency. Please do not use other than the specified voltage.
3. Do not damage, modify, pull, over bend or twist the power cord, do not place heavy objects on the power cord.
4. Do not place the product on unstable workbenches, such as shaky tables, bevels, or vibrations.
5. Keep the scaler clean before and after operation. The scaling tip, wrench and handpiece (detachable) must be sterilized before each treatment.
6. The tip must be tightened to the handpiece with torque wrench. While scaler is working, the heat of scaling tip may become higher if there is no water flowing out, make sure the irrigation is good.
7. Don't twist or rub the tip. Change a new one when the tip is damaged or worn excessively.
8. Don't screw the scaling tip while stepping on the foot switch.
9. Don't use impure water source, and be sure not to use normal brine instead of pure water source.
10. If use the water source without hydraulic pressure, the water surface should be one meter higher than the head of the patient.
11. Don't knock or rub the handpiece. Do not pull the cable while the device is working, to avoid damage to the cable.
12. After operating, turn off electrical source, and then pull out the plug.
13. The screw thread of the scaling tips produced by other manufacturers is maybe coarse, rusty and collapsed, which will damage the screw thread of the handpiece irretrievably. Please use our scaling tip.
14. This equipment is only applicable to the corresponding type of power adapter produced by our company.
15. As a professional manufacturer of medical instruments, we are only responsible for the safety on the following conditions:
 - The maintenance, repair and modification are made by the manufacturer or the authorized dealer.
 - The changed components are original of our company and operated correctly according to instruction manual.
16. This product is intended for use in hospitals and dental clinics only. The user must be professionally trained and qualified dentists.
17. Indicator light: Other colours: Meaning other than red, yellow, or green, indicated the device ready for use.
18. Statement: the third conductor in the POWER SUPPLY CORD is only a functional earth.

Symbol instruction

Symbol	Instruction	Symbol	Instruction	Symbol	Instruction
	Caution	H_2O 0.01MPa-0.5MPa	Water entrance pressure:0.01MPa-0.5MPa		Earth (ground)
	Recovery	IPX1	Protected against dripping water		Sterilizable in a steam sterilizer (autoclave) at 134°C
	Date of manufacture		Manufacturer		For indoor use only
	Class II equipment		Type B applied part		Alternating current
	ON (power)		OFF (power)	ON/OFF	Switch power on/off
	Adjustment for the water flow		Adjustment for the power		Foot switch interface
	Mode of LED		Mode of outside-water system		Mode of bottle-water system
	Temperature limit: -20°C- +40°C		Atmospheric pressure limitation: 70kPa-106kPa		Humidity limitation: 10%-93%
	Keep dry		Fragile, handle with care		Waste electrical and electronic equipment
	Consult instructions for use		Authorized representative in the European Community		

1 Product introduction

1.1 Product overview

Guilin Refine Medical Instrument Co.,Ltd. is a professional manufacturer to research, develop, produce and sell ultrasonic scalers. The product is used for teeth cleaning and also an important device for teeth disease prevention and treatment. The Ultrasonic scaler is composed of main unit, handpiece, cable, water pipe, tip, torque wrench, foot switch, and power supply.

The ultrasonic scaler has following features:

- a) Circular vibration orbit, scaling and polishing together.
- b) Small vibrating amplitude, enjoy the painless treatment.
- c) Titanium scaling tips, no injury to cementum.
- d) Clinical solutions are applicable for automatic water supply mode, including Hydrogen peroxide, sodium hypochlorite, chlorhexidine.
- e) LED Handpiece, LED mode and non-led mode available, better visibility.
- f) Automatic frequency tracking ensures that the machine always works on the best frequency and more steadily.
- g) Digital control, easy operation and more efficient for scaling.
- h) The silicon-cover can be autoclaved to high temperature 134°C and high pressure 0.22Mpa.

1.2 Contraindications:

- 1) The hemophilia patient is forbidden to use this equipment.
- 2) The patients or doctors with heart pacemaker are forbidden to use this equipment.
- 3) The heart disease patient, pregnant woman and children should be cautious to use the equipment.

1.3 Equipment safety classification

- 1) Operating mode: Continuous operation
- 2) Type of protection against electric shock: Class II
- 3) Degree of protection against electric shock: Type B applied part
- 4) Applied part of the equipment: Tip
- 5) Degree of protection against harmful ingress of water: Ordinary equipment
- 6) Degree of protection against harmful ingress of water: protection degree against water (used on foot switch): IPX1
- 7) Degree of safety of application in the presence of a flammable anesthetic mixture with air or with oxygen or nitrous oxide: Equipment can not be used in the presence of a flammable anesthetic mixture with air or with oxygen or nitrous oxide

1.4 Model and technical Parameters

Table 1: Technical Parameters

Parameters	PT 7
Size (mm)	270mm*255mm*135mm
Weight of main unit	2.5Kg


Parameters	PT 7
Handpiece model	HY-1L
Touch control	YES
Water bottle	With
Rated input	220-230V AC 50Hz / 110V AC 60Hz
Input Power	38VA
Fuse of main unit	T0.5AL 250V
Primary tip vibration excursion	1 μ m-200 μ m
Tip vibration frequency	28kHz-42kHz
output power of tip	3W-20W
half-excursion force	0.1N-2N
Water entrance pressure	0.01MPa-0.5MPa

1.5 Working condition


- 1) Environment temperature: +5°C-+40°C
- 2) Relative humidity: 30%-75%
- 3) Atmosphere pressure: 70kPa-106kPa
- 4) Temperature of the water at the inlet: not higher than +25°C

2 Installation and adjustment

2.1 Product installation steps

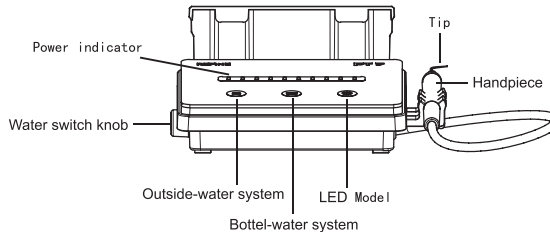

Picture 1. Front of the main unit sketch map

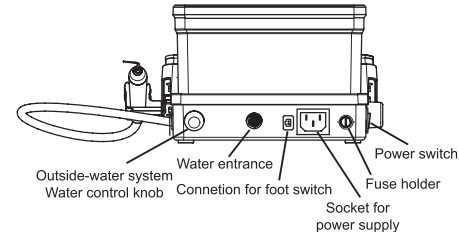

Picture 2. Back of the main unit sketch map

2.1.1 Unpack the package, make sure that all the parts and accessories are complete according to the packing list, take the main unit out of the box, and put it on the stable plane facing to the operator.

2.1.2 Turn the water control knob to the max, Do not screw it over tight in case of damage.

2.1.3 Insert the plug of the foot switch to the socket.

2.1.4 Connect one end of the water pipe to the water entrance, and the other end to the clean water source.

2.1.5 Connect the handpiece (detachable) to the cable.

2.1.6 Install the tip on the handpiece and turn on the power switch to start operation.

2.2 Instruction for main components of detachable handpiece (showed in picture 3).

a) Nipple: The Nipple can be removed. You can screw out the Nipple and clean the pole with alcohol termly.

b) Handpiece: The main part of the whole handpiece, can be autoclaved under the high temperature and pressure.

c) Light pipe, LED lamp: Clean them with purified water and sterilize them under the high temperature of 134°C and high pressure of 0.22Mpa.

d) The connector of the cable: Connect the handpiece with the water source and power supply of the main unit.

 Note: The connection of handpiece and the plug must be kept dry.

2.3 Assemble and disassemble the tip using the wrench


a) The torque wrench's structure is designed in special way which can control the strength of the scaling tip installation properly and correctly. It also can guarantee the operator screw or unscrew the scaling tip effectively and keep their hands away from being scratched.

b) Operation

- Take the tip into the torque wrench then install or uninstall the scaling tip as picture 3 showed.

- Installation: Hold the handpiece and turn the tip toward clockwise direction with the torque wrench. Turn one more circle when the tip stops, then the tip is installed.

- Uninstallation: Hold the handpiece, turn the wrench toward anti-clockwise direction.

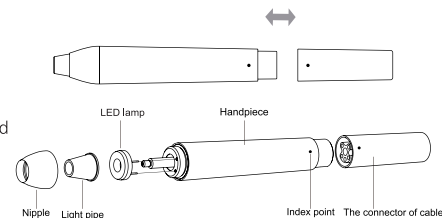

Picture 3

3 Scaling & periodontal treatment function and use

3.1 Install the product correctly according to the product installation steps, and the operator is facing the machine. Turn on the power switch, the power indicator lighted and the machine is ready for work.

3.2 Using the touch panel, the machine can directly touch the water supply mode identification or power size indicator on the panel to select the water supply mode or adjust the power size.

3.3 Choose the scaling tip according to the requirement, and fix the scaling tip with the wrench. (see picture 4) Please select a suitable power when using different type of tips.

3.4 Press the foot switch, the tip vibrates, and the LED lamp at the top of the handpiece lights up. When the foot switch is released, the LED lamp continues to light up for 10 seconds and then goes out.

3.5 Select whether LED lamp mode is needed according to clinical needs. Click the key to switch on or off the LED lamp when the handpiece is working.

3.6 The handpiece can be handled in the same gesture as a pen in hand.

3.7 Under normal working condition, the frequency of the tip is very high, light touch and a certain to-and-fro motion will eliminate the tartar without obvious heating, overexertion and overstay are forbidden.

3.8 Vibrating intensity: Adjust the vibrating intensity according to your need, usually adjust to the middle grade, and adjust the vibrating during the clinical treatment according to the patient's sensitivity and the rigidity of the tartar.

3.9 Water volume adjustment: Step on the foot switch, and the tip begins to vibrate, then turn the water control switch to fine spray to cool down the handpiece and clean the teeth.

3.10 During clinical cleaning, please keep the side of the tip in contact with the tooth surface at zero degree angle, without applying pressure, so that the tip can vibrate freely.

3.11 Step on the foot switch, the tip begins to vibrate, and the LED lamp on the top of the handpiece lights up. Release the foot switch, the LED lamp keep shining for 10 seconds.


3.12 After finishing operation, keep the machine working for 30 seconds with the water supply to clean the handpiece and the tip.

3.13 Unscrew the scaling tip and sterilize it.

3.14 flushing: under the bottled water system mode, adjust the water volume to the maximum, and step on the foot to enter the flushing mode.

⚠️ Note: Be sure not to make the end of the tip touch the teeth vertically, and not use too much force when the tip touching the surface of the teeth, in case of hurting the teeth and damaging the tip.

⚠️ Note: Don't screw the scaling tips when stepping on the foot switch, while the machine is working.

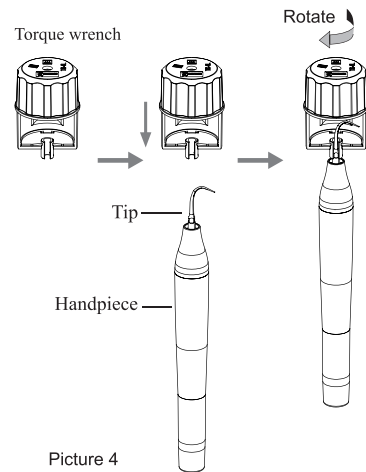

Picture 4

4 Troubles shooting

4.1 Troubles shooting list

Fault	Possible	Solutions
The scaling tip doesn't vibrate and no water flowing out when stepping on the foot switch.	The plug is in loose or wrong contact.	Connect the power plug well.
	The foot switch is in loose contact.	Connect the switch well.
	The fuse is broken.	Change a new fuse.

Fault	Possible	Solutions
The scaling tip doesn't vibrate, but there is waterflowing out when stepping on the foot switch.	The scaling tip is in loose contact.	Screw it tightly (see picture 4)
	The connector plug of the handpiece with the circuit board is in loose contact.	Contact with the local distributor or manufacturer.
	Malfunction of the handpiece.	Contact with the local distributor or manufacturer.
The scaling tip vibrates but there is no spray come out when stepping on the foot switch.	The water control switch is off.	Turn on the switch [note 1].
	There is impurity in the solenoid valve.	Contact with the local distributor or manufacturer.
	The water pipe is jammed.	Clean water pipe by multi-function syringe [note 2].
There is water flow out when turn off the power.	There is impurity in the solenoid valve.	Contact with the local distributor or manufacturer.
The handpiece generates heat.	The amount of spouting water is too little.	Turn the water control switch to a higher grade [note 1].
	The potentiometer is broken.	Change a new one.
The amount of spouting water is too little.	The water control knob is a low grade.	Turn the knob to a high grade [note 1].
	The water pressure is not enough.	Enhance the water pressure.
	The water pipe is jammed.	Clean the water pipe by multi-function syringe [note 2].
The vibration of the tip becomes weak.	The tip hasn't been screwed tightly or becomes loose because of vibration.	Screw the scaling tip tightly (picture 4).
	The tip is damaged.[note 3]	Change a new one.
	The tip is damaged [note 3].	Change a new one.
The vibrating intensity control knob is seized up.	The potentiometer is damaged.	Contact with the local distributor or our company.

If the troubles still can't be solved, please contact with the local distributors or manufacturer.

4.2 Notice

[Note 1] The water control knob can adjust the water volume according to the image.

[Note 2] To clean the water pipe with the multi-function syringe of the dental unit (see picture 4):

a) Snip the water pipe at a distance of 10cm to 20cm from the water entrance.

- b) Turn on the power switch, get through to the power.
- c) Connect the multi-function syringe of the dental unit to the water pipe.
- d) Screw off the scaling tip or pull out the handpiece.
- e) Step on the foot switch.
- f) Turn on the switch of the multi-function syringe, press the air or water into the water pipe to clean and eliminate the impurity.

[Note 3] If the scaling tip has been screwed on tightly and there is fine spray too, the following phenomena show that the scaling tip is damaged:

- a) The vibrating intensity and the pulverization degree become weak obviously.
- b) During operating, there is some buzz when the scaling tip is working.


5 Cleaning, disinfecting and sterilizing

5.1 Please conform to the recommendations of the manual "Reprocessing Instructions of Cleaning, Disinfecting And Sterilizing" delivered with your product regarding the procedure of cleaning, disinfecting, sterilizing and packing of the components. Follow present-day regulations enforced in the country about reprocessing. The use of scouring powder or an abrasive sponge will damage its surface.

5.2 The handpiece, scaling tips, torque wrench, LED lamp and Light pipe can be sterilized.

Notice:

- a) Clean the handpiece with compressed air before sterilization.
- b) Be sure that the scaling tip has been unscrewed from the handpiece and it cannot be sterilized with others.
- c) Please notice whether the outer of the handpiece is damaged during the treatment and sterilization. Don't smear any protective oil on the surface of handpiece.
- d) There are two waterproof "O" rings at the end of the handpiece. Please lubricate them with dental lube frequently, as sterilization and repeated pulling and inserting will reduce their using life. Change a new one once it is damaged or worn excessively.
- e) The following sterilizing methods are forbidden:
 - Boil in water.
 - Dip in iodine, alcohol and glutaraldehyde.
 - Bake in oven or microwave oven.

 **Notice:** We are not responsible for any damage caused in the above items.

6 Transportation, Storage And Maintenance

6.1 Transportation

- 6.1.1 Excessive impact and shake should be prevented in the transportation. Lay it carefully and lightly and don't invert it.
- 6.1.2 Don't put it together with dangerous goods during transportation.
- 6.1.3 Avoid solarization and getting wet in rain or snow during transportation.

6.2 Storage

6.2.1 Don't store the machine together with the articles that are combustible, poisonous, caustic, or explosive.

6.2.2 This equipment should be stored in a room where the relative humidity is 10%-93%, atmospheric pressure is 70kPa-106kPa, and the temperature is -20°C-+40°C.

6.3 Maintenance

6.3.1 The equipment should be handled carefully and lightly. Be sure that it is far from the vibration, and installed or kept in a cool, dry and ventilated place.

6.3.2 Please turn off the electrical source if not use it, if not use for a long time, please make the machine get through to the power and water once 3 months for five minutes.

7 Environmental protection

Please dispose according to the local laws.

8 EMC - Declaration of conformity

8.1 Instructions for use

The ME EQUIPMENT or ME SYSTEM is suitable use in hospitals or dental clinics.


Warning: Don't near active HF surgical equipment and the RF shielded room of an ME system for magnetic resonance imaging, where the intensity of EM disturbances is high.

Warning: Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

Warning: Use of accessories, transducers and cables other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.

Warning: Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the equipment, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

Note: The emissions characteristics of this equipment make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required) this equipment might not offer adequate protection to radio-frequency communication services. The user might need to take mitigation measures, such as relocating or re-orienting the equipment.

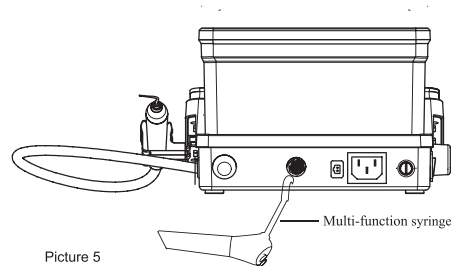

List of all cables

No	Name	Length	Shielded or not	Detachable or not	Note
1	Power Cord	2.0m	No	Yes	/
2	Foot Switch Cord	2.5 m	No	Yes	/
3	Ultrasonic Scaler Handpiece Cord	2.0 m	No	No	/

Replaceable accessories

No	Name	Model	Connection method	Note
1	Ultrasonic Scaler Handpiece	HY-1L	plug	/
2	Foot Switch	/	plug	/
3	Ultrasonic Scaler Tip	Refer to Packing list	/	/
4	Power cord	/	/	/
5	Torque wrench	TW-5L	/	/
6	Autoclavable box	/	/	/

Performance of the me equipment

PT 7 Ultrasonic Scaler is suitable for periodontal treatment in oral clinical treatment, which can remove dental calculus and plaque on the supragingival and subgingival, and achieve the therapeutic effect of improve periodontal tissue; The product uses the TL494 pulse width modulated chip of Texas Instruments (TI) as the ultrasonic pulse generator, and use STM8S003 control processor of STMicroelectronics. The processor searches for the working frequency point of the transducer by controlling the change of ultrasonic frequency and makes it vibrate harmoniously with the scaler tip. When the me equipment essential performance is ineffective or degraded due to em disturbances, the doctor should immediately stop using it to ensure that there is no treatment error. And then remove the source of disturbances or adjust the direction or position of me equipment to ensure me equipment can be used in normal performance condition.

8.2 Technical description

8.2.1 Portable and mobile RF communications equipment may affect the performance of equipment , use of equipment should be avoided strong electromagnetic interference, and do not closer to mobile phone, microwave oven, etc.

8.2.2 Use of equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

8.2.3 Except for the transducer and cables sold by manufacturers of as spare parts of internal components, the use of handpiece cables and accessories other than those specified or provided by the manufacturer may result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.

8.2.4 Use of accessories, transducers, handpiece and cables other than those specified or provided by the manufacturer together with equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.

8.2.5 The PT 7 Ultrasonic Scaler uses RF energy only for its internal functions. Therefore, it has low RF emissions and is less likely to cause interference to nearby electronic equipment.

Guidance and manufacturer's declaration -electromagnetic emissions and Immunity

Table 1

Guidance and manufacturer's declaration - electromagnetic emissions	
Emissions test	Compliance
RF emissions CISPR 11	Group 1
RF emissions CISPR 11	Class A
Harmonic emissions IEC 61000-3-2	Not Applicable
Voltage fluctuations / flicker emissions IEC 61000-3-3	Not Applicable

Table 2

Guidance and manufacturer's declaration - electromagnetic Immunity		
Immunity test	IEC 60601 test level	Compliance level
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±2 kV, ±4 kV, ±8 kV, ±15 kV air	±8 kV contact ±2 kV, ±4 kV, ±8 kV, ±15 kV air
Electrical fast transient/burst IEC 61000-4-4	±2 kV power supply lines ±1 kV signal input/output 100 kHz repetition frequency	±2 kV power supply lines Not applicable 100 kHz repetition frequency
Surge IEC 61000-4-5	±0.5 kV, ±1 kV differential mode ±0.5 kV, ±1 kV common mode	±0.5 kV, ±1 kV differential mode Not applicable
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	0 % UT; 0,5 cycle. At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315°. 0 % UT; 1 cycle and 70 % UT; 25/30 cycles; Single phase: at 0°. 0 % UT; 250/300 cycle	0 % UT; 0,5 cycle. At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315°. 0 % UT; 1 cycle and 70 % UT; 25/30 cycles; Single phase: at 0°. 0 % UT; 250/300 cycle
Power frequency magnetic field IEC 61000-4-8	30A/m 50Hz/60Hz	30A/m 50Hz/60Hz
Conducted RF IEC61000-4-6	3 V 0,15 MHz – 80 MHz 6 V in ISM bands between 0,15 MHz and 80 MHz 80 % AM at 1 kHz	3 V 0,15 MHz – 80 MHz 6 V in ISM bands between 0,15 MHz and 80 MHz 80 % AM at 1 kHz
Radiated RF IEC61000-4-3	3 V/m 80 MHz – 2,7 GHz 80 % AM at 1 kHz	3 V/m 80 MHz – 2,7 GHz 80 % AM at 1 kHz

NOTE U_i is the a.c. mains voltage prior to application of the test level.

Table 3

Guidance & Declaration - Electromagnetic immunity						
Radiated RF IEC61000-4-3 (Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communications equipment)	Test Frequency (MHz)	Band (MHz)	Service	Modulation	IEC 60601-1-2 Test Level (V/m)	Compliance level (V/m)
	385	380 – 390	TETRA 400	Pulse modulation 18 Hz	27	27
	450	430 – 470	GMRS 460, FRS 460	FM ± 5 kHz deviation 1 kHz sine	28	28
	710	704 – 787	LTE Band 13, 17	Pulse modulation 217 Hz	9	9
	745					
	780					
	810	800 – 960	GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation 18 Hz	28	28
	870					
	930					
	1720	1700 – 1990	GSM 1800; CDMA 1900; GSM 1900; DECT; LTE Band 1, 3, 4, 25; UMTS	Pulse modulation 217 Hz	28	28
	1845					
	1970					
	2450	2400 – 2570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation 217 Hz	28	28
	5240	5100 – 5800	WLAN 802.11 a/n	Pulse modulation 217 Hz	9	9
5500						
5785						

Table 4

Guidance and manufacturer's declaration - electromagnetic Immunity				
Radiated RF IEC61000-4-39 (Test specifications for ENCLOSURE PORT IMMUNITY to proximity magnetic fields)	Test Frequency	Modulation	IEC 60601-1-2 Test Level (A/m)	Compliance level (A/m)
	30 kHz	CW	8	8
	134,2 kHz	Pulse modulation 2.1 kHz	65	65
	13,56 kHz	Pulse modulation 50 kHz	7,5	7,5

Attachment. Reprocessing instructions of cleaning, disinfecting and sterilizing

1. Beginning Work!

1.1 Please read these operating instructions carefully as they explain all the most important details and procedures. Please pay special attention to the safety precautions. Always keep this instruction close at hand.

1.2 To prevent injury to people and damage to property, please heed the corresponding directives.

1.3 The instructions in this manual are only applicable to the product which it was delivered with.

2. Introduction

2.1 These reprocessing instructions provide instructions for cleaning, disinfection, sterilization and packaging of manufacturer reusable products intended to be reprocessed in medical facilities.

2.2 The goal of reprocessing reusable products is to reduce bioburden and to achieve sterility of those products in order to eliminate the risk of product reuse related infection. Decisions regarding cleaning, disinfecting or sterilizing manufacturer's medical and dental products are based on the potential risk of infection associated with their use.

2.3 It is recommended to use steam sterilization.

2.4 Remember that sterilization or high-level disinfection cannot be achieved unless the elements of the assembly are cleaned first.

2.5 If you find that the reprocessing instructions from the manufacturer seem to be inadequate, please inform manufacturer about those inadequacies.

2.6 We encourage you to report adverse events related to device reprocessing. Report such events directly to manufacturer.

3. Reprocessing - Instructions For Reusable Products

3.1 The instructions are binding for the reprocessing of all reusable products (Here

after called "products") of manufacturer. When necessary, additional product-specific instructions are included with the product to provide additional information.

! Important: Before use, carefully read the operating instructions of the manufacturer instrument and devices with which the product will be used.

3.2 Reusable products must be cleaned, disinfected and sterilized prior to first use. Reprocessing procedures have only limited implications to this device. The limitation of the numbers of reprocessing procedures is therefore determined by the function / wear of the device. From the processing side there is no maximum number of allowable reprocessing. The device should no longer be reused in case of signs of material degradation.

! In case of damage the product should be reprocessed before sending back to the manufacturer for repair.

4. Preparation - Basic Principles

4.1 It is only possible to carry out effective sterilization after the completion of effective cleaning and disinfection. Please ensure that, as part of your responsibility for the sterility of products during use, only sufficiently validated equipment and product-specific procedures are used for cleaning/disinfection and sterilization, and that the validated parameters are adhered to during every cycle.

4.2 Please also observe the applicable legal requirements in your country as well as the hygiene regulations of the hospital or clinic. This applies especially with regard to the additional requirements for the inactivation of prions.

5. Preparation at the Point of Use

Disconnect product. Remove gross soiling of the instrument with cold water (<40°C) immediately after use. Don't use a fixating detergent or hot water (>40°C) as this can cause the fixation of residuals which may influence the result of the reprocessing process.

Store the products in a humid surrounding.

6. Transportation

Safe storage and transportation to the reprocessing area to avoid any damage and contamination to the environment.

7. Preparation for Decontamination

The products must be reprocessed in a disassembled state, as far as possible.

8. Pre-cleaning

Do a manual pre-cleaning, until the products are visually clean. Submerge the products in a cleaning solution and flush the lumens with a water jet pistol with cold tap water for at least 10 seconds. Clean the surfaces with a soft bristle brush.

9. Cleaning


Regarding cleaning/disinfection, rinsing and drying, it is to distinguish between manual and automated reprocessing methods. Preference is to be given to automated reprocessing methods, especially due to the better standardizing potential and industrial safety.

Automated Cleaning:

Use a washer-disinfector (WD) meeting the requirements of the ISO 15883 series. Put the instrument into the machine on a tray. Connect the instrument with the WD by using suitable adapter and start the program:

- 4 min pre-washing with cold water (<40°C);
emptying
- 5 min washing with a mild alkaline cleaner at 55°C
emptying
- 3 min neutralising with warm water (>40°C);
emptying
- 5 min intermediate rinsing with warm water (>40°C)
Emptying

The automated cleaning processes have been validated by using 0.5% neodisher MediClean forte (Dr. Weigert).

 Acc. to EN ISO 17664 no manual reprocessing methods are required for these devices. If a manual reprocessing method has to be used, please validate it prior to use.

10. Disinfection

Automated Thermal Disinfection in washer/disinfector under consideration of national requirements in regards to A0 value (see EN 15883).

A disinfection cycle of 5 min disinfection at 93°C has been validated for the product to achieve an A0 value of 3000.

11. Drying:

Automated Drying:

Drying of outside of instrument through drying cycle of washer/disinfector. If needed, additional manual drying can be performed through lint free towel. Insufflate cavities of products by using sterile compressed air.

12. Functional Testing, Maintenance

Visual inspection for cleanliness of the products and reassembling if required. Functional testing according to instructions of use. If necessary, perform reprocessing process again until instrument is visibly clean.

Before packaging and autoclaving, make sure that the products have been maintained acc. to manufacturer's instruction.

13. Packaging

Pack the products in an appropriate packaging material for sterilization. The packaging material and system refer to EN ISO 11607.

14. Sterilization

Sterilization of products by applying a fractionated pre-vacuum steam sterilization process (according to EN 285/EN 13060/EN ISO 17665) under consideration of the respective country requirements.

Minimum requirements: 3 min at 134 °C (in EU: 5 min at 134 °C)

Maximum sterilization temperature: 138°C

Drying time:

For steam sterilization, we recommend a drying time of 15 to 40 minutes. Choose a suitable drying time, depending on the autoclave and load. Refer to the autoclave's instructions for use.

After sterilization:

- a. Remove the product from the autoclave.
- b. Let the product cool down at room temperature for at least 30 minutes. Do not use additional cooling.

Check that the sterilization wraps or pouches are not damaged.

⚠ Flash sterilization is not allowed on lumen instruments.

⚠ The manufacturer assumes no responsibility for the use of other sterilization procedures (e.g. ethylene oxide, formaldehyde and low temperature plasma sterilization). In such cases, please observe the respective valid standards (EN ISO 14937/ANSI AAMI ISO 14937 or the procedure-specific standard) and verify the suitability and effectiveness in principle of the procedure (if necessary, including investigations on sterilizing agent residue), taking into account the specific product geometry as part of the validation.

15. Storage

Storage of sterilized products in a dry, clean and dust free environment at modest temperatures, refer to label and instructions for use.

16. Service Life

The products have been designed for a large number of sterilization cycles. The materials used in their manufacture were selected accordingly. However, with every renewed preparation for use, thermal and chemical stresses will result in aging of the devices. If the number of permissible re-sterilization cycles is restricted, this will be pointed out in the product specific instructions.

⚠ The use of ultrasound baths and strong cleaning and disinfection fluids (alkaline pH>9 or acid pH<5) can reduce the life span of devices. The manufacturer accepts no liability in such cases.

⚠ The devices may not be exposed to temperatures above 138 °C.

It is the duty of the user to ensure that the reprocessing processes including resources, materials and personnel are capable to reach the required results. State of the art and often national law requiring these processes and included resources to be validated and maintained properly.

Note: We reserve the rights to change the design of the equipment, the technique, fittings, the instruction manual and the content of the original packing list at any time without notice. If there are some differences between blueprint and real equipment, take the real equipment as the norm.

Shelf life: 10 years, the date of manufacture see product label.



Guilin Refine Medical Instrument Co., Ltd.

No.8-3, Information Industrial Park, High-Tech Zone,
Qixing District, Guilin, Guangxi, 541004, P.R. China
Tel: +86-773-7796686 Email:refine@refine-med.com
Website: <http://www.refine-med.com>



MedNet EC-REP GmbH
Borkstrasse 10 · 48163 Muenster · Germany



MediMap Ltd
2 The Drift Thurston Suffolk IP31 3RT United Kingdom

Scan and Login website for
more information

